


Electrical diagrams R-net

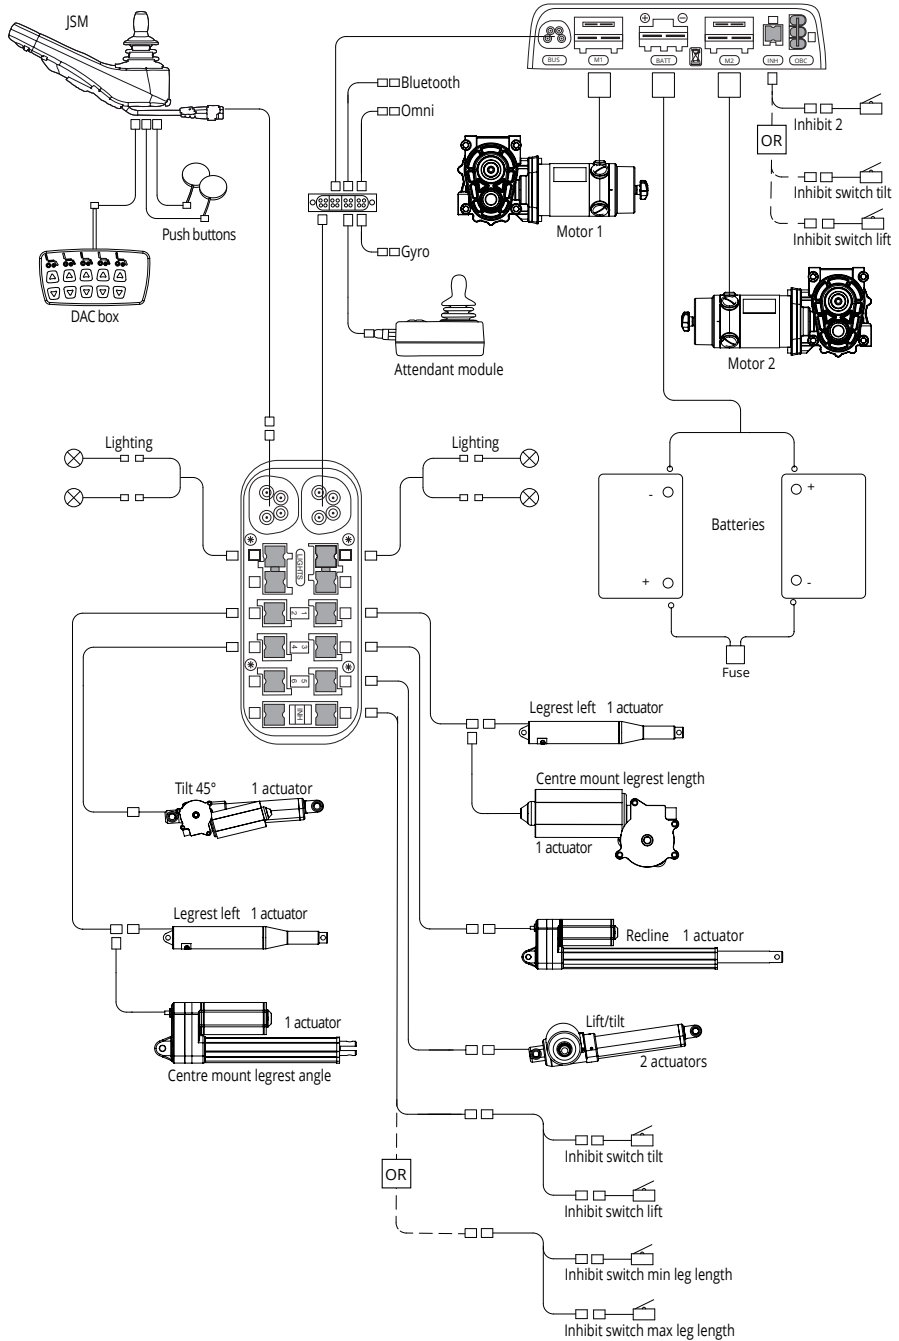

Connect the batteries

See figure 23 how to connect the battery charger.

The controller includes a '3-pin connection'. Ensure that the battery charger is properly connected so that the 'negative pole' and the 'inhibit' are connected, enabling the system to prevent the wheelchair from moving when the battery is being charged (figure 24).

